


Product Overview



A	Gauge Face
B	Hose
C	Pressure Indicator Needle
D	Suggested Pressure Zone
E	Pressure Relief Valve
F	Bulb
G	Internal Bladder
H	Finger Cuff

Specifications

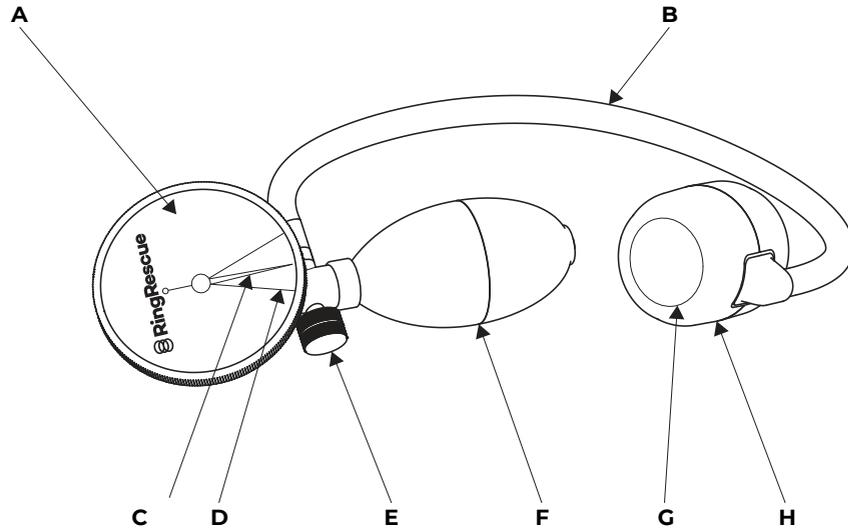

**Warning**

ALWAYS consult labeling that accompanies accessories for instructions on proper use and storage.

**Caution**

ALWAYS store this equipment within the specified environmental limits described in this manual.


**Note**

Specifications are approximate and may vary between devices

<b>Model:</b>	Ring Rescue® Compression Device™ RDC-A1-UC
<b>Mass:</b>	0.23 KG (0.51 lb)
<b>Maximum Finger Diameter:</b>	25.5 mm (1.0 in)

Environmental Conditions:	Operation	Transportation and Storage
Ambient Temperature Limitation		
Relative Humidity		
Atmospheric Pressure		

Technical Reference Manual

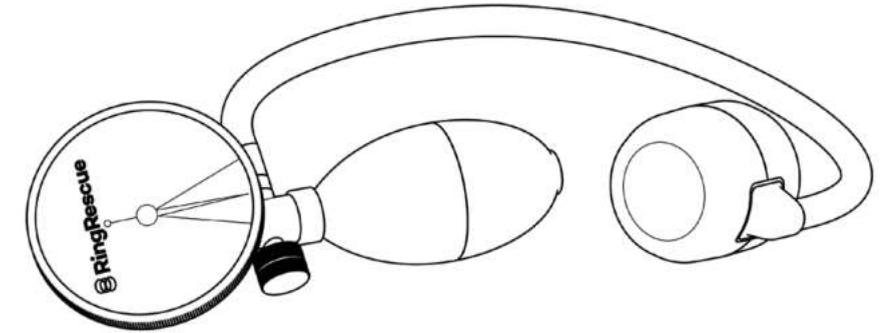

Ring Rescue® | CompressionDevice™



## Ring Rescue® | Compression Device™



RDC-A1-UC

FEI Number: 3015542886

Health Canada MDEL Number: 9115

US Patent: 10,702,282



Ring Rescue Inc.  
20 Orion Court  
Dartmouth, Nova Scotia  
Canada  
B2Y 4W6  
1 (888) 640-7464  
ringrescue.com



Made In Canada with domestic and imported parts

### Introduction

This Technical Reference Manual represents the most up-to-date knowledge pertaining to the safe and effective use of the Ring Rescue® Compression Device™. This manual is intended to be used by trainers, nurses, physicians, and technicians. Always keep a reference of this manual available for consultation during the life of the product. Before using this product, please consult the provided *Quick Start Guide* and become familiar with its operation by watching the instructional videos at:

[ringrescue.com/tutorial](http://ringrescue.com/tutorial)

or by scanning the QR code below and watching the instructional videos.



### Background

The Ring Rescue® Compression Device™ uses air pressure to temporarily compress a swollen finger, allowing for the removal of an entrapped finger ring. Ring removal techniques are then needed to remove the ring.

### Indications for use

The Ring Rescue® Compression Device™ is indicated for use when a ring is stuck on a finger (ring entrapment), and removal is desired. The device, along with correct ring removal techniques, will often enable the removal of stuck rings.

### Directions for use

Before using this product, please consult the Ring Rescue® Compression Device™ *Quick Start Guide* as well as the instructional videos available at:

[ringrescue.com/tutorial](http://ringrescue.com/tutorial)

### Contraindications For Use

Do not use in cases of severe finger injury.

### Definitions

The symbols located on the equipment and/ or labeling are defined in this section or in the *Symbol Definition Chart*. See the *Symbol Definition Chart* supplied with the equipment.

Symbol	Definition
	General warning sign
	Read instructions before use

### Caution

Do not exceed 15 minutes of total compression time. Seek qualified medical advice in cases where finger bone fracture, nerve/vascular injury, skin laceration or damage, or injured ligaments and tendons are suspected.



### Warning

Use only Ring Rescue® approved accessories and components (such as Ring Rescue® Ring Lubricant™) with this product. DO NOT modify this product or its accompanying accessories in any way. Modifications to this device or its accessories will void the warranty and may cause damage or harm.

### Cleaning Instructions

Before and after each use, clean the device and its components with 70% alcohol or 0.5% accelerated hydrogen peroxide wipes. Do not use any other cleaning substances or chemicals. Do not

submerge any components in liquid. Keep device out of direct sunlight or ultraviolet light.

It is recommended a medical glove be applied over the affected hand during device use to preserve cleanliness.

### Tutorials

Scan the QR code or visit the link below for Ring Rescue® Compression Device™ instructional videos:



[ringrescue.com/tutorial](http://ringrescue.com/tutorial)

### Product Expiry

Consult the product label, located on the backside of the gauge face, for device manufacture and expiry information.

### Warranty

When operated and maintained according to all instructions supplied, if the Ring Rescue® Compression Device™ fails due to a defect in material or workmanship within one (1) year from the date of original retail purchase, the product will be repaired or replaced at the option of Ring Rescue Inc. for no additional charge. This warranty does not cover unsuccessful ring removal attempts. For full details see [www.ringrescue.com/warranty](http://www.ringrescue.com/warranty)